



TIMING DEFIBRILLATION SHOCKS IMPROVES DEFIBRILLATION SUCCESS

Harold M. Hastings¹, Teri Whitman², Steven J. Evans³, Flavio Fenton¹, Alan Garfinkel⁴, Jagannathan Geetha¹
 1. Hofstra University, 2. Medtronic, Inc., 3. Beth Israel Medical Center, 4. UCLA School of Medicine

BACKGROUND

Although cardiac electrical activity in ventricular fibrillation (VF) is apparently highly disordered, Damle et al.¹ and Bayly et al.² found strong evidence for local spatial organization, paving the way for extensive further investigation. Garfinkel et al.³ characterized VF as spatio-temporal chaos, finding underlying dynamic order. Gray, Pertsov and Jalife⁴ and Witkowski et al.⁵ demonstrated the existence of multiple spirals in VF. More recently, Bayly et al. quantified⁶ spatial correlation in VF by demonstrating a correlation length of 4-10 mm.

If a degree of organization and periodicity exists during VF, perhaps the current required to defibrillate could be reduced if the shock were delivered at an optimum point in the fibrillatory cycle. Perhaps if the shock were delivered during a during a time period when a large portion of the myocardium is depolarized or refractory, then less current would be required to depolarize an additional portion of the myocardium to reach a critical mass for defibrillation. Finally, defibrillation at such a time in the cardiac cycle might minimize the chances that VF would reinitiate following defibrillation (cf. refs 7,8).

PURPOSE AND HYPOTHESIS


Purpose: reduce defibrillation threshold for practical, implantable defibrillators

Hypothesis: defibrillation threshold can be reduced by timing with respect to spatio-temporal data

Limitations imposed in clinical practice:

- Small number of allowed sensing electrodes
- Limited computational power
- Structure of waveforms - see below
- Baseline variability and drift
- Amplitude variability

TYPICAL WAVEFORMS (unipolar electrograms)

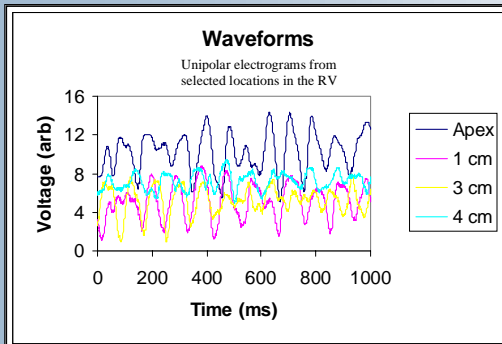

SUMMARY

Study Goals

To determine whether success of defibrillation can be improved by suitably timing defibrillation shocks. Current internal defibrillators synchronize the shock to an activation measured from an RV tip bipole.

Methods

In a prospective study directed by Teri Whitman of Medtronic, four isoflurane-anesthetized pigs were instrumented with a Medtronic 6944 true bipolar lead in the RV apex, a diagnostic catheter in the great cardiac vein, and a subcutaneous patch in the pectoral region. In addition, a 2-8-2 mm diagnostic catheter was placed along the RV free wall for the retrospective study described herein. Fibrillation was induced with a T shock and defibrillation was attempted after 10 seconds of VF using one of four synchronization methods: 1) asynchronous, or synchronized to the first sensed activation from 2) RV tip/ring electrogram (EGM), 3) RV coil/sub-cutaneous patch EGM, or 4) LV bipolar EGM. Twenty sets of 4 shocks were given at energies stepping around the overall 50% successful defibrillation dose. The retrospective study analyzed voltages and slew rates recorded by the RV diagnostic catheter in order to determine whether success of defibrillation can be improved by suitably timing defibrillation shocks. 317 of the 320 recordings were usable.

Results

The number of sites in the repolarizing state was correlated with defibrillation success (success: 1.66 ± 0.08 ; failure 1.38 ± 0.08 (mean \pm SEM), $p=0.016$, paired t-test). Moreover, defibrillation was significantly more successful when the both the apex and most distant site were in the repolarizing state (65% vs. 51%, chi-squared = 4.88, $p < 0.05$). This criterion was met 26 % of the time. Finally, in a preliminary estimate with logistic regression, applying this criterion appears to reduce defibrillation energy by 19 (+12, -9) %.

Conclusions

Retrospective analysis indicates that defibrillation success could be significantly improved by sensing two sites in the RV and delivering shocks when both sites are in the repolarizing state.

The future

Modeling study to optimize criteria of this type in two ways: maximizing the reduction in defibrillation energy and minimizing the expected waiting time until the criterion is met. Design a prospective animal experiment aimed at a 40% reduction in defibrillation energy, and perform that animal experiment.

Selecting a criterion

Look at successes and failures
 Study behavior of electrograms

Unipolar electrograms at the apex and 4 cm distal
 Average number of sites in depolarization

	Average	Standard Dev	SEM
Failures (n = 145)	0.96	(0.40)	(0.029)
Successes (n = 171)	0.86	(0.40)	(0.03)
Difference	0.10		(0.045)

$t = 2.41, p = 0.016$

Evaluating the criterion

Consider how often criterion met
 and effect upon defibrillation success

Criterion: Apex and 4 cm distal both repolarizing

How often met ? 26 % of time


Criterion met ?	Successes	Failures	Trials	Prob. of success	Std Error
No	121	115	236	51.3%	3.3%
Yes	53	28	81	65.4%	5.3%
Total	174	143	317	54.9%	2.8%

Chi-squared = 4.84, $p < 0.05$

IMPROVED DEFIBRILLATION SUCCESS

Effects of selected criterion upon defibrillation

Data fit with logistic regression (SAS 6.12), maximal likelihood fit, inter-animal differences modeled by Boolean variables

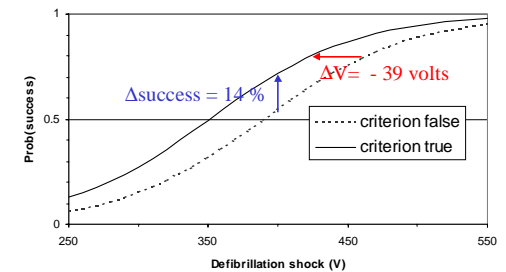

BIBLIOGRAPHY

- Bayly PV, Johnson EE, Wolf PD, et al. A quantitative measure of spatial order in ventricular fibrillation. *J Cardiovasc Electrophysiol* 4:533-546, 1993.
- Damle RS, Kanaan NM, Robinson NS, et al. Spatial and temporal linking of epicardial activation directions during ventricular fibrillation in dogs: Evidence for underlying organization. *Circulation* 86:1547-1558, 1992.
- Garfinkel A, Walter DO, Chen P-S et al. Quasi-periodicity and chaos in cardiac fibrillation. *J Clin Investigation* 99:305-314, 1997.
- Gray RA, Pertsov AM and Jalife J. Spatial and temporal organization during cardiac fibrillation. *Nature* 392:75-78, 1988.
- Witkowski FX, Leon LJ, Postawa PA, et al. Spatiotemporal evolution of ventricular fibrillation. *Nature* 392:78-82, 1988.
- Bayly PV, KenKnight BH, Rogers JM, et al. Spatial organization, predictability and determinism in ventricular fibrillation. *Chaos* 8:103-115, 1998.
- Chen P-S, Wolf PD, Ikker RE. Mechanism of cardiac defibrillation: A different point of view. *Circulation* 84:913-919, 1991.
- Skoubine K, Tseyanova N, Moore P. Success and failure of defibrillation shock: Insights from a simulation study. *J Cardiovasc Electrophysiol* 11:785-796, 2000.
- Jones JL, Klein GJ. Ventricular fibrillation: The importance of being coarse? *J Electrocardiol* 17:393-400, 1984.
- Kuehl KW, Hsia P, Wise RM, Mahmud R, Damiano RJ. Integration of absolute ventricular fibrillation voltage correlates with successful defibrillation. *IEEE Trans Biomed Eng* 41:782-790, 1994.
- Hsia PE, Frenk S, Allen CA, Wise RM, Cohen NM, Damiano RJ. A critical period of ventricular fibrillation more susceptible to defibrillation: Real-time waveform analysis using a single ECG lead. *PACE* 19:418-430, 1996.
- Hsia PE, Suresh G, Allen CA, et al. Improved nonbarocatheter defibrillation based on ventricular fibrillation waveform characteristics. *PACE* 19:1537-1547, 1996.
- Guramathan S, Hsia P, Lawton J, Hsu D. Vector magnitude using orthogonal ECG leads during ventricular fibrillation is associated with defibrillation outcome. *Biomed Instrum Technol* 32:48-61, 1998.
- Parwardhan A, Moghe S, Wang K, Cruise H, Leonelli F. Relation between ventricular fibrillation voltage and probability of defibrillation shocks: Analysis using Hilbert Transforms. *J Electrocardiol* 31:313-325, 1998.
- Carlisle EJJ, Allen JD, Bailey A, et al. Fourier analysis of ventricular fibrillation and synchronization of DC countershocks in defibrillation. *J Electrocardiol* 21:337-343, 1988.
- Hsu W, Lin Y, Heil JE, Jones J, Lang DJ. Effect of shock timing on defibrillation success. *PACE* 20(Pt 11): 153-157, 1997.
- Hsu W, Lin Y, Lang DJ, Jones JL. Shock timing lowers transvenous defibrillation energy requirement. *J Electrocardiol* 31 (Supp):35-40, 1998.
- Hsu W, Lin Y, Jones JL, Lang DJ. Transvenous defibrillation efficacy is improved for shocks critically timed to characteristics in endocardial morphology but not surface electrograms. *PACE* 20 (Pt II): 1167, 1997.
- Hsu W, Lin Y. Ventricular defibrillation by coordination of shocks with sensed coarse VF complexes. US Patent 5,632,766, May 27, 1997.
- Hsu W, Lin Y, Lang DJ, Jones JL. Improved internal defibrillation success with shocks timed to the morphology electrogram. *Circulation* 98:808-812, 1998.
- Hsu W, Lin Y, Zhu A, Jones JL, Lang DJ. Shocks timed to the morphology electrogram lower defibrillation threshold and sharpen probability of success curves. *PACE* 20 (Pt 11): 1167, 1997.
- Jones J, Torar O, Hsu W. Shock synchronization to fibrillation action potential repolarization reduces and stabilizes defibrillation threshold. *PACE* 22:720, 1999.
- Jones J, New WA, Moulden JC, et al. Synchronized shocks reduce defibrillation threshold. *Proc IEEE EMBS* 19:145-147, 1997.
- Hsu W, Lin Y, Lang DJ, Jones J. Shocks synchronized to activations in low intensity regions of the ventricle decrease defibrillation threshold. *PACE* 21:791, 1998.
- Li HG, Yee R, Mehra R, DeGroot P, Klein GJ, Zardini M, Thakar RK, Morillo CA. Effect of shock timing on efficacy and safety of internal cardioversion for ventricular tachycardia. *J Am Coll Cardiol* 24:703-708, 1994.
- Wandeker S, Kay GN, KenKnight BH, et al. The effects of ventricular fibrillation duration and a preceding unsuccessful shock on the probability of defibrillation success using biphasic waveforms in pigs. *J Cardiovasc Electrophysiol* 8:1386-1395, 1997.
- Roberts P, Allen S, Smith D, et al. Defibrillation efficacy after failed defibrillation. *PACE* 21:972, 1998.